


# hydrorise system

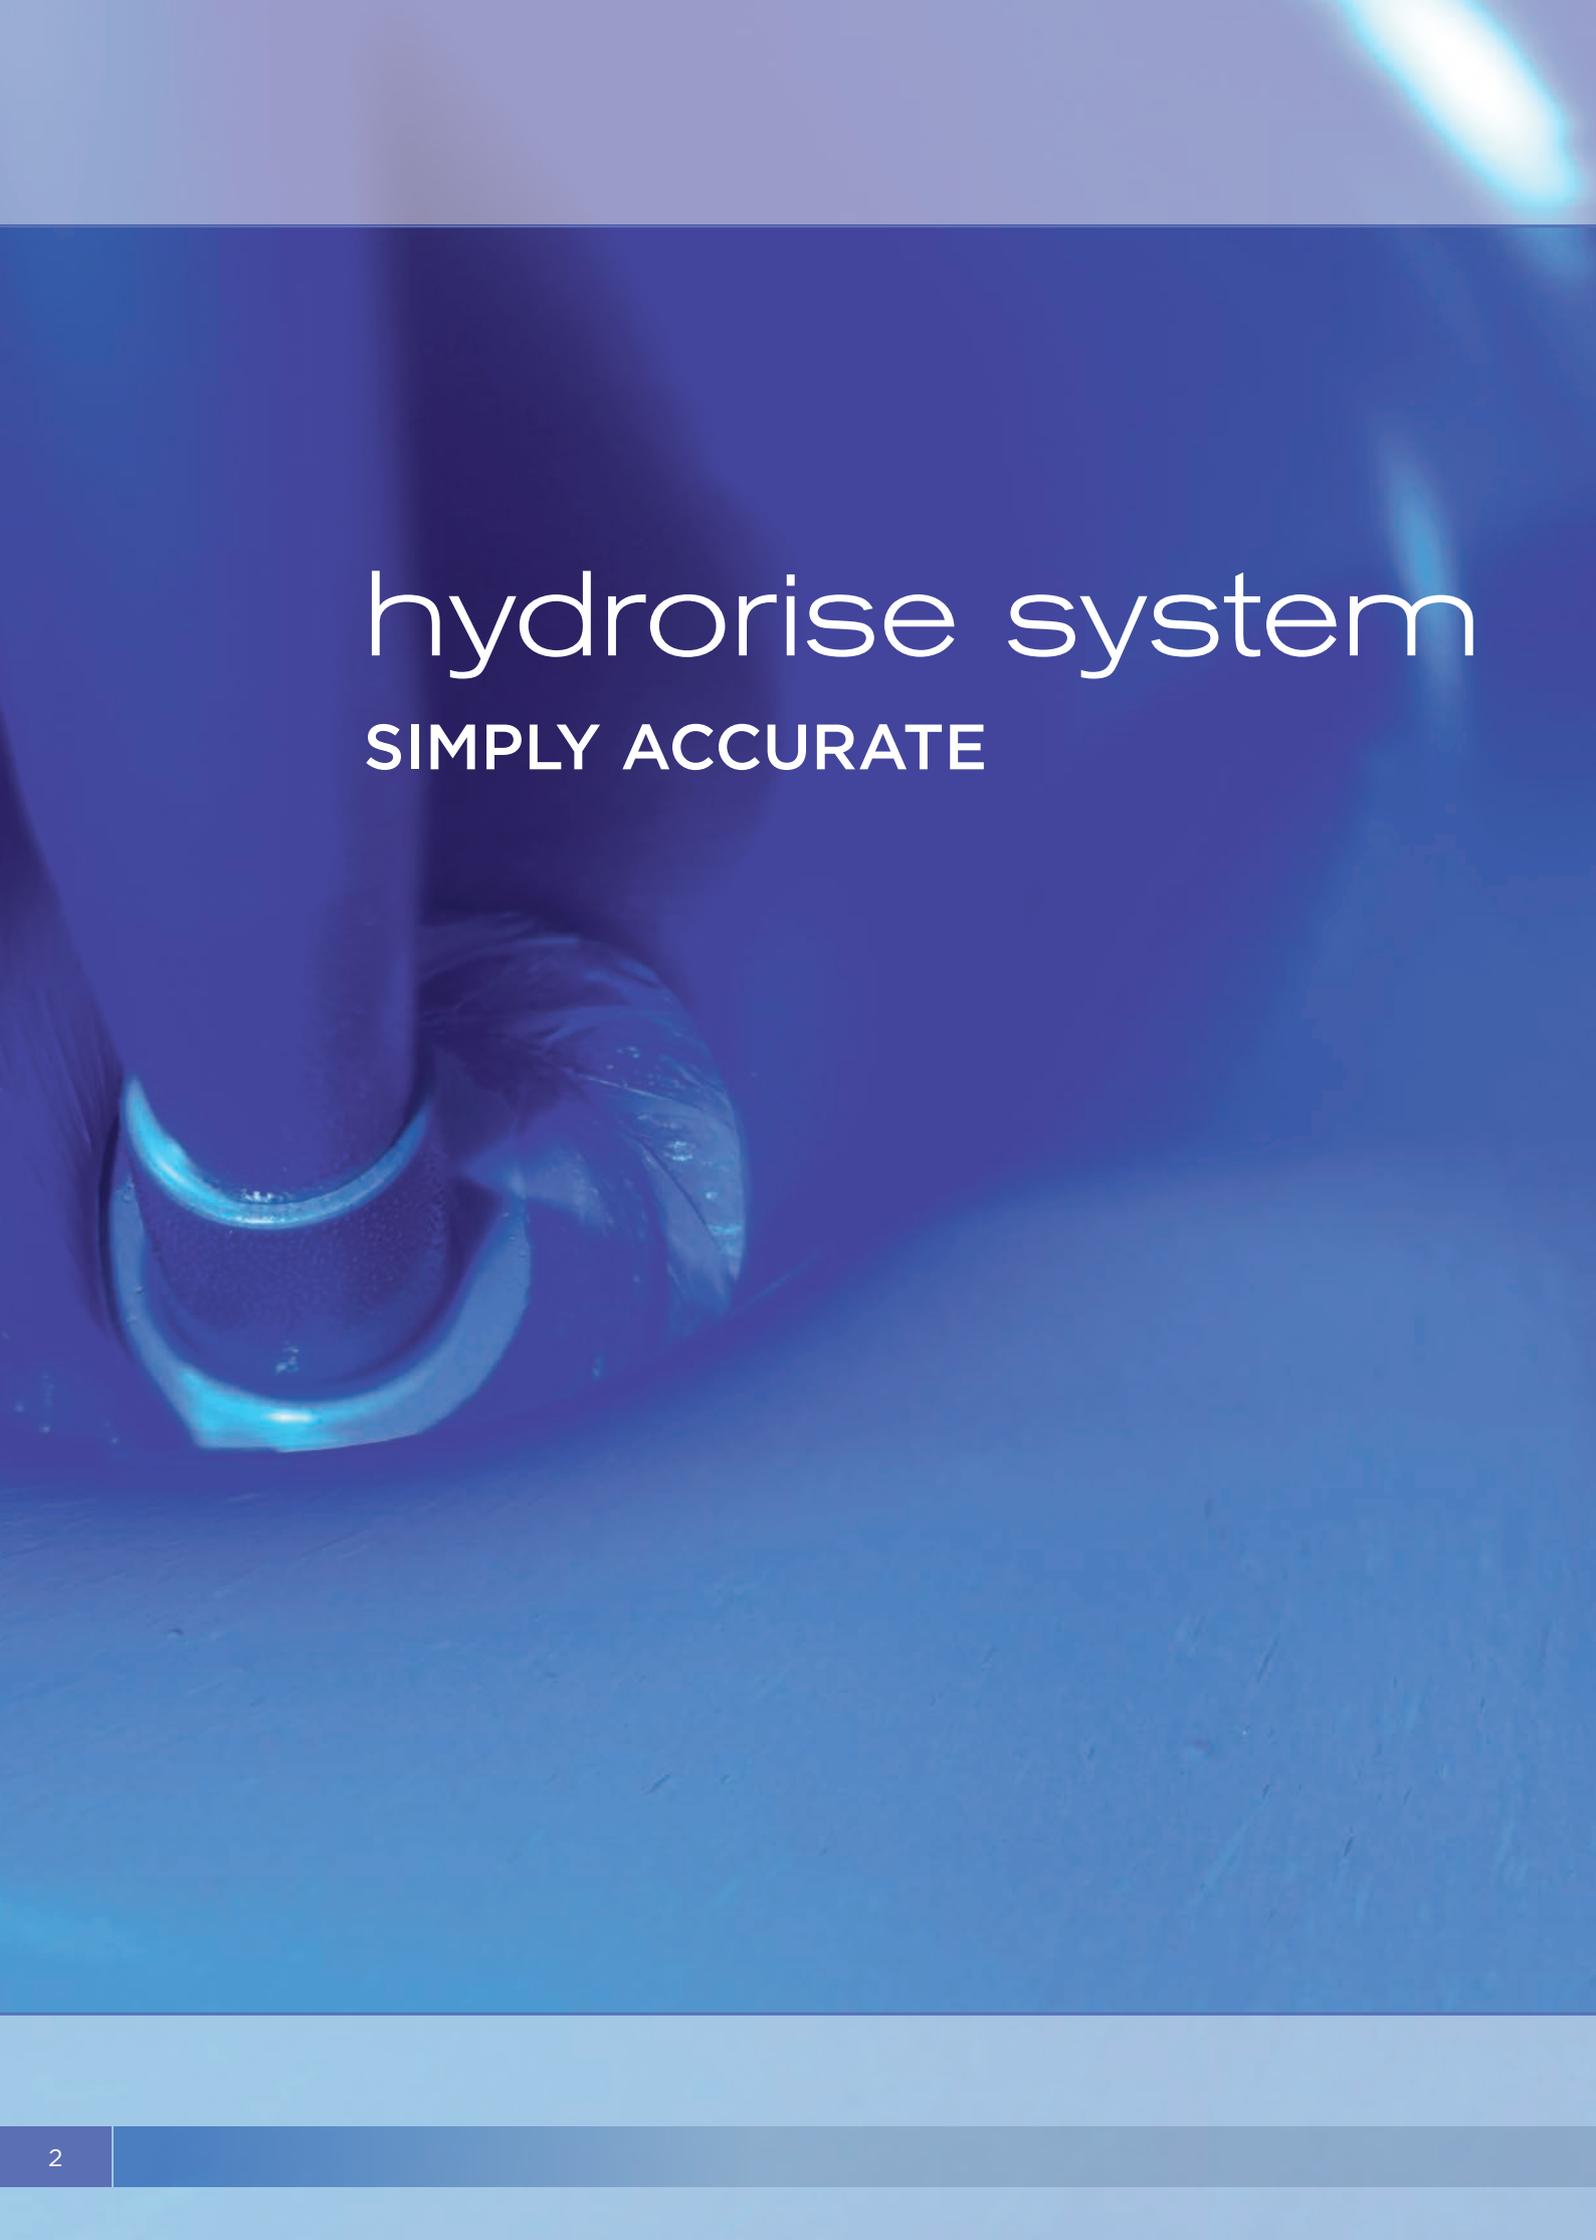

## SIMPLY ACCURATE

Addition silicones for impression taking

A close-up photograph of a hand using a tool to work on a pipe, with a blue overlay. The hand is wearing a blue glove and is using a tool to work on a pipe. The background is a solid blue color.

# hydrorise system

**SIMPLY ACCURATE**

# Hydrorise Implant and Hydrorise, two key components of Hydrorise System. With one single objective: accuracy.

## A SYSTEM THAT STANDS OUT FOR ACCURACY AND RELIABILITY

**Hydrorise System** is a complete range of addition silicones for impression taking, formulated for professionals seeking high performance solutions. Hydrorise System is the **top of the Zhermack range** and guarantees **accuracy** and **reliability**.

## TWO KEY COMPONENTS. ONE RANGE.

Hydrorise System delivers the precision and accuracy that the professional needs, for impressions of implants and of natural abutments. **Hydrorise Implant** is scannable and has high rigidity for implant impression taking. **Hydrorise** also guarantees fine detail reproduction which, combined with excellent hydrocompatibility, contributes to the precision and accuracy of natural abutment impressions.

## THE FULL RANGE Zhermack product choice guide

HIGH-TECH,  
HIGH-PERFORMANCE  
SOLUTIONS

**extraPro**

Hydrorise System

SOLUTIONS  
FOR SPECIFIC  
APPLICATIONS

**specialPro**

VERSATILE  
SOLUTIONS

**multiPro**

ESSENTIAL  
SOLUTIONS


**easyPro**

hydrorise implant



**ONE SINGLE OBJECTIVE.**

hydrorise

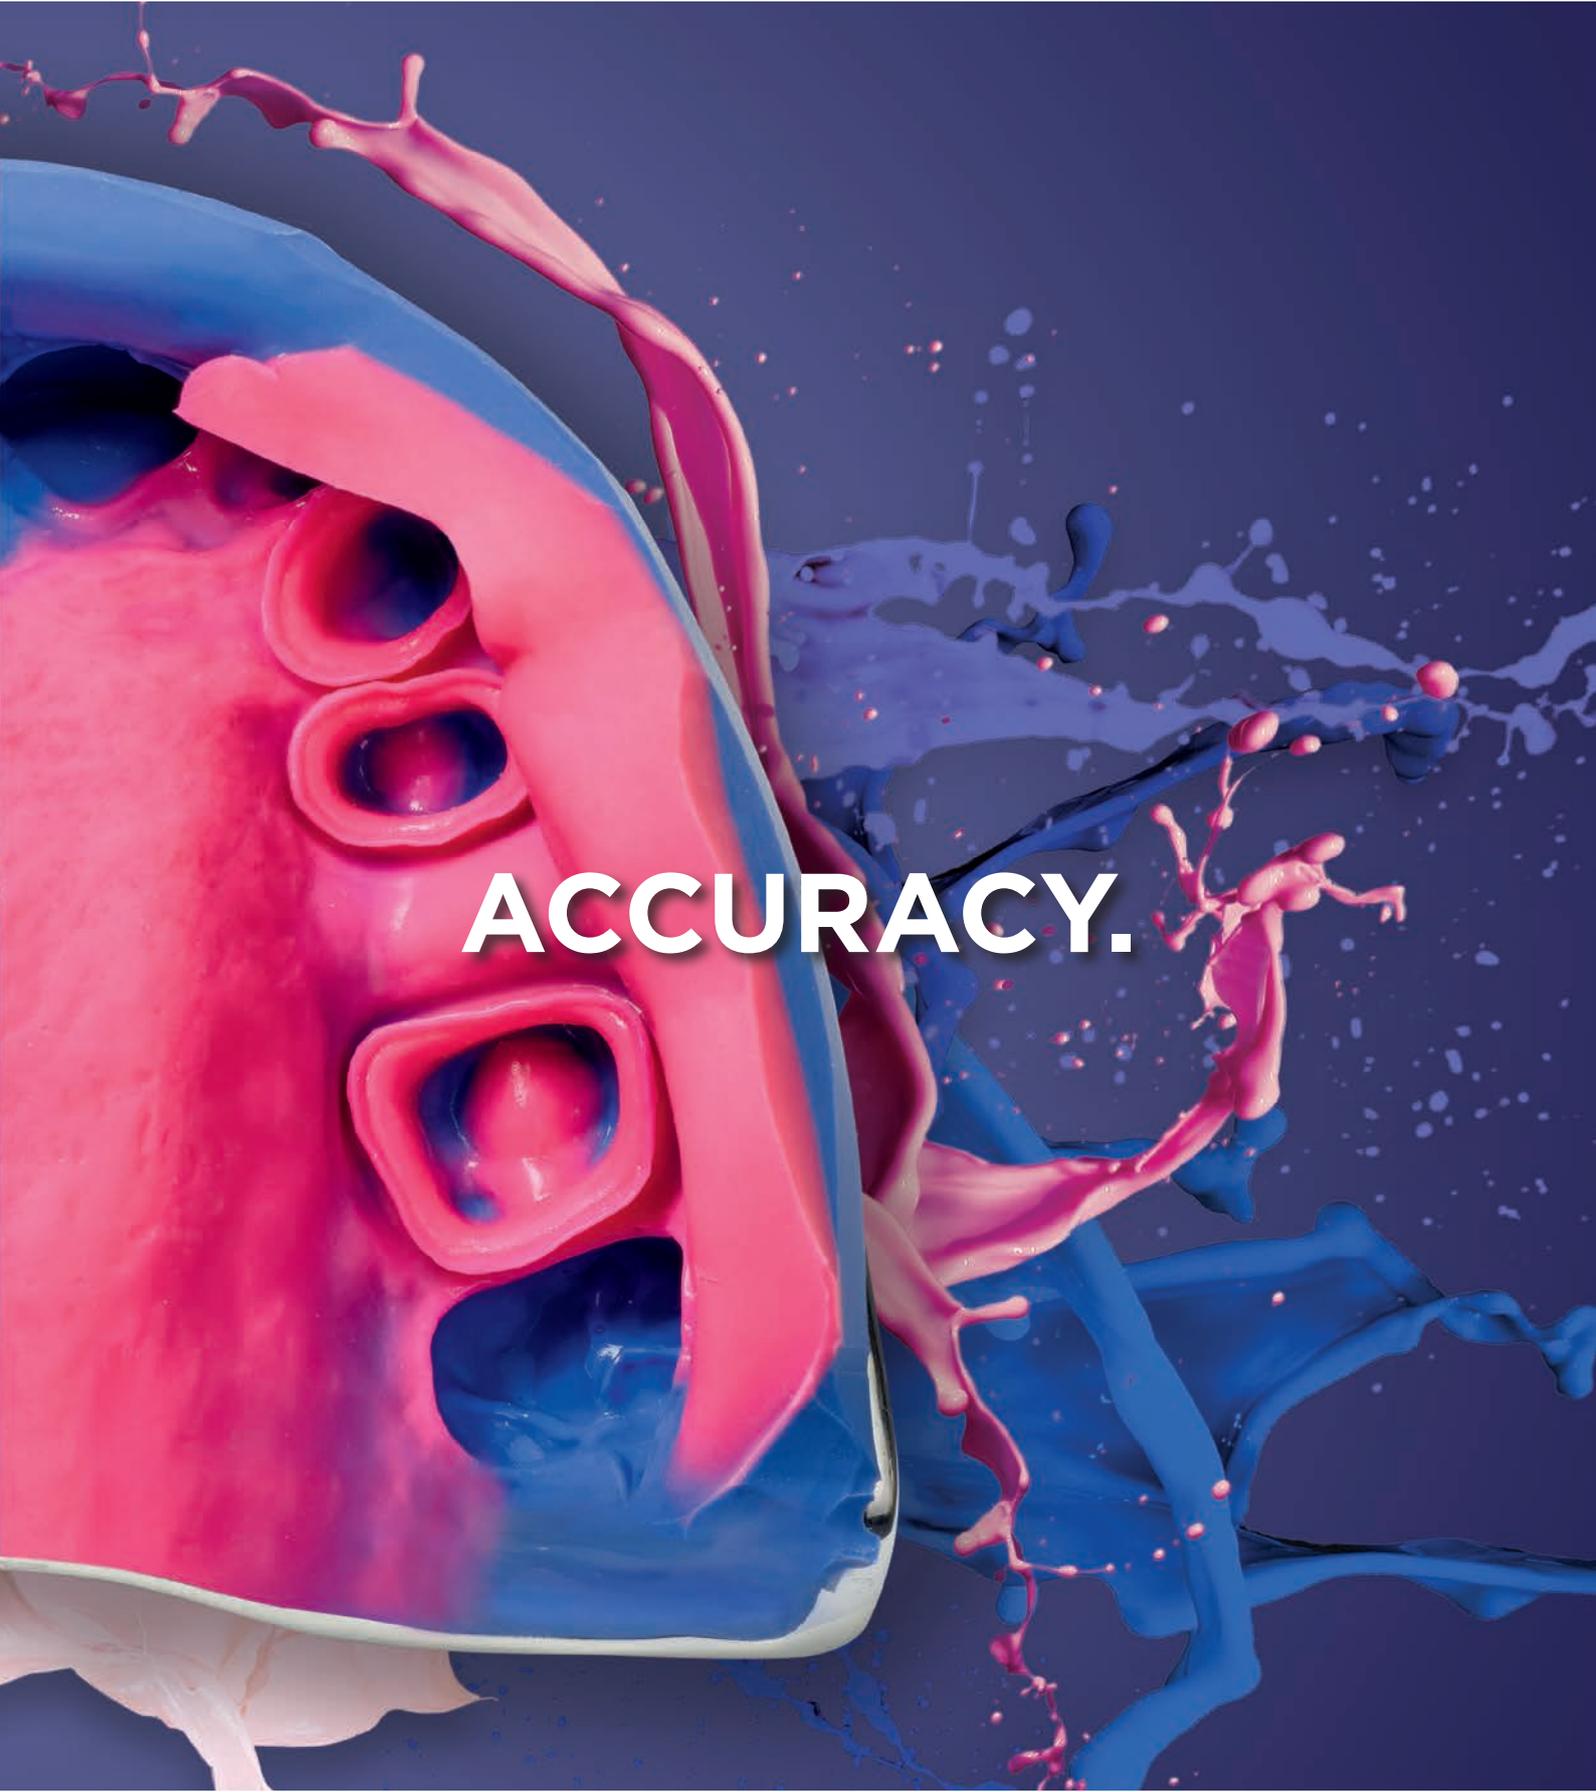

**ACCURACY.**

A close-up photograph of a dental handpiece, which is a metal tool used for preparing teeth. The handpiece is held by a hand wearing a blue nitrile glove. The handpiece is positioned over a dental model, which is a replica of a patient's teeth. The background is a dark blue gradient. The text "WITH HYDRORISE IMPLANT IMPRESSIONS ARE RIGHT FIRST TIME." is overlaid on the left side of the image.

WITH **HYDRORISE IMPLANT**  
IMPRESSIONS ARE RIGHT  
FIRST TIME.



## FORMULATED FOR IMPLANT PROSTHODONTICS

Hydrorise Implant is a scannable addition silicone **with high rigidity**, formulated for implant prosthodontics.

The greater rigidity of Hydrorise Implant viscosities compared to those of Hydrorise achieves greater stability in transfers to impressions. It also ensures that the correct three-dimensional position is maintained even after removal from the oral cavity.<sup>[1]</sup>

## HIGH RIGIDITY AND ELASTICITY IN PERFECT BALANCE

To take impressions of implants, material must have ideal rigidity<sup>[2]</sup> while being sufficiently **elastic** to permit easy extraction from the oral cavity. Thanks to their elasticity, VPS can be considered the impression material of choice in these cases, especially in the presence of angulated implants<sup>[3]</sup>.

# Hydrorise Implant

FOCUS

## TESTED RELIABILITY

Hydrorise Implant has all the characteristics needed to satisfy the latest requirements in implant prosthodontics.

A recent in vitro study, **undertaken by the Universities of Bologna and Padua**, showed that Hydrorise Implant offers **significantly greater accuracy** and **precision** than polyethers: even under unfavourable conditions with unsplinted transfers, its performance is similar or better than that of the polyethers tested.<sup>[1]</sup>





## SCANNABILITY


Hydrorise Implant combines high-performance technical properties with the benefits of digital workflows. Thanks to its unique formula, Hydrorise Implant **is scannable** even without reflective sprays. The scannability of impressions **facilitates access to digital workflows** without requiring the use of an intraoral scanner. It also reduces the risk of errors caused by the casting of traditional gypsum models.

## RADIOPACITY: A HYDRORISE IMPLANT EXCLUSIVE\*

**Radiopacity** allows dentists to identify any subgingival material residues with a plain-film X-ray performed in the dental practice, thus affording the professional peace of mind and ensuring patient comfort.

\* Within the Zhermack product portfolio



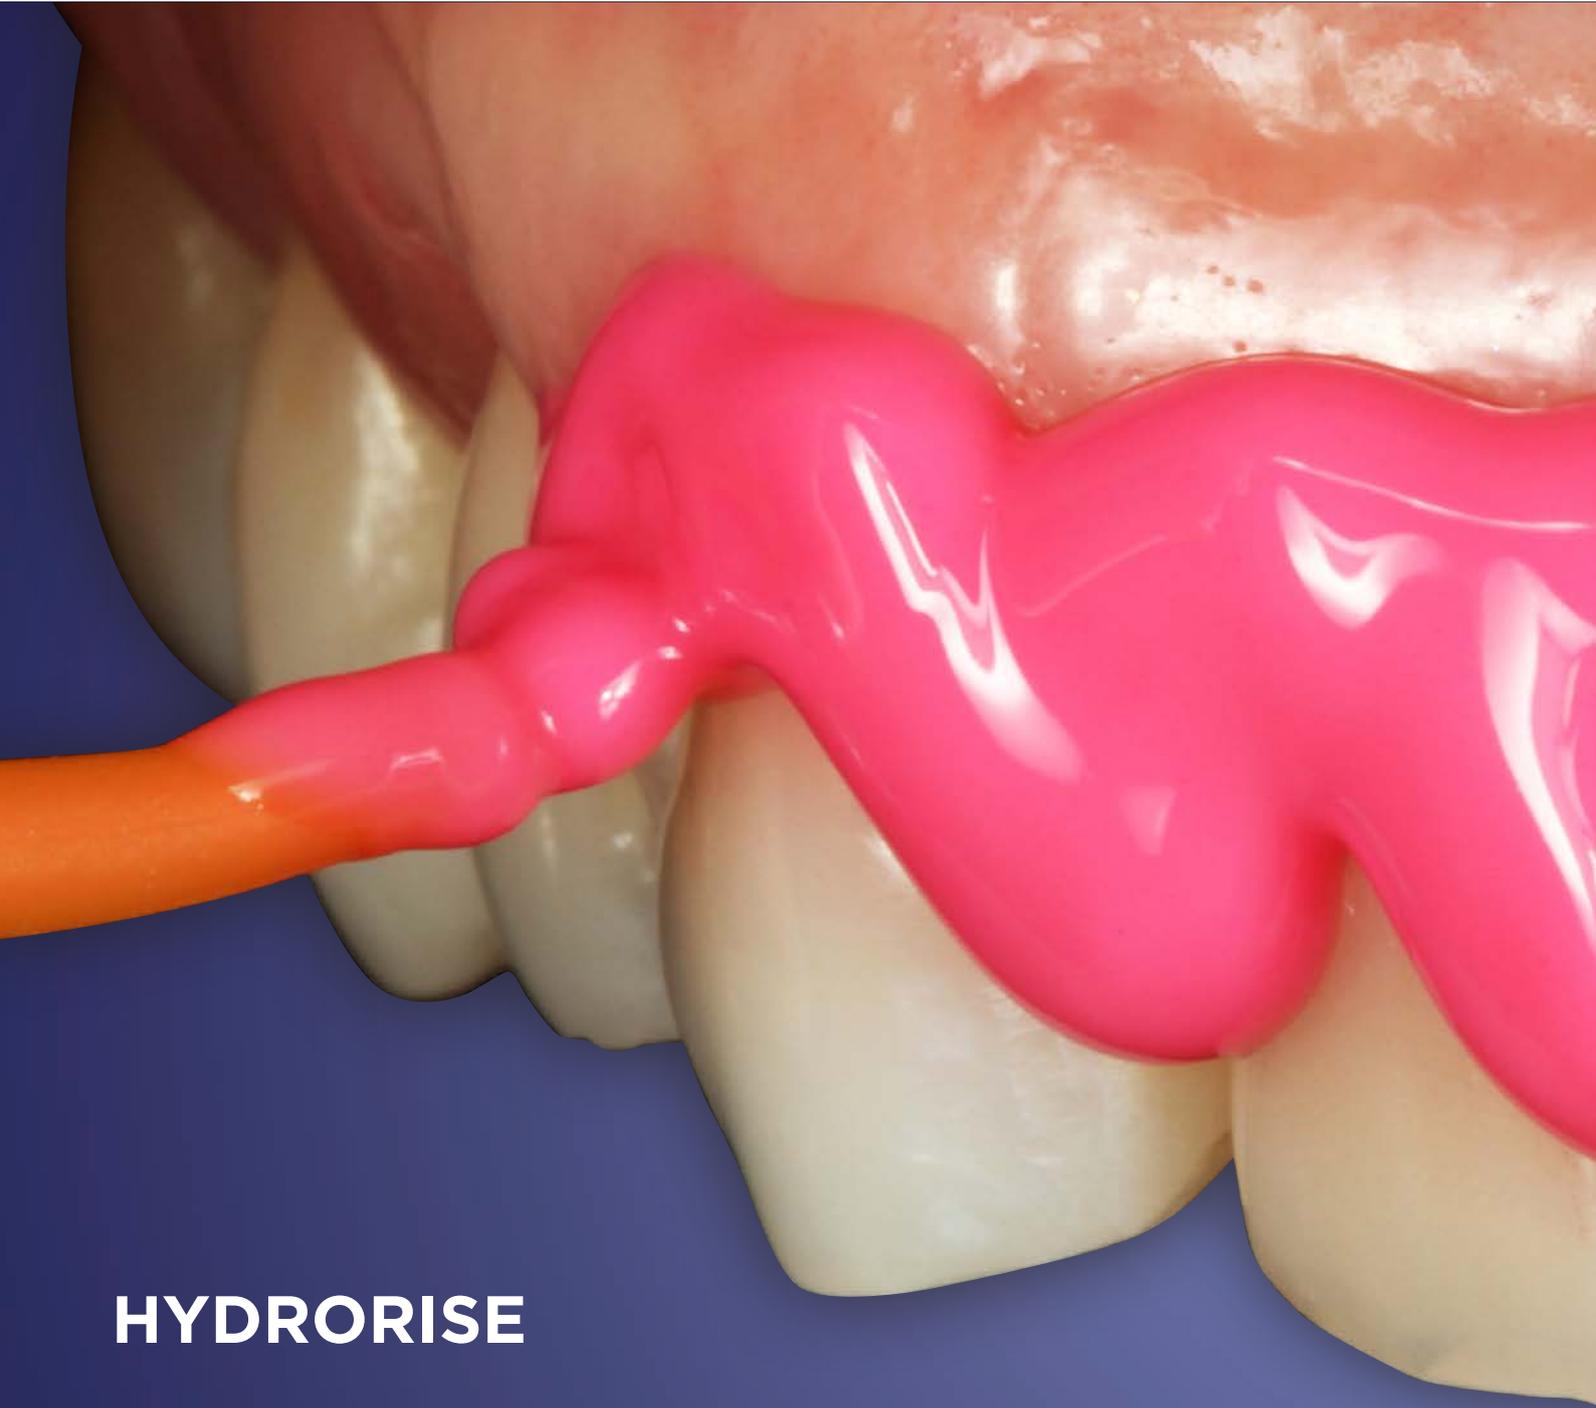

## **HYDRORISE**

WHAT IS PRECISION  
MADE OF?




## DETAILS MAKE THE DIFFERENCE

Hydrorise addition silicone guarantees **excellent detail reproduction.**

Adequate detail reproduction is one of the main requirements for a successful impression.<sup>[4]</sup> Zhermack has developed a product that goes well beyond **applicable standards** with **precision 4 times greater** than that demanded by European standards.\*

Hydrorise fluids offer a precision of **5 microns**, ensuring excellent detail reproduction.

# Hydrorise

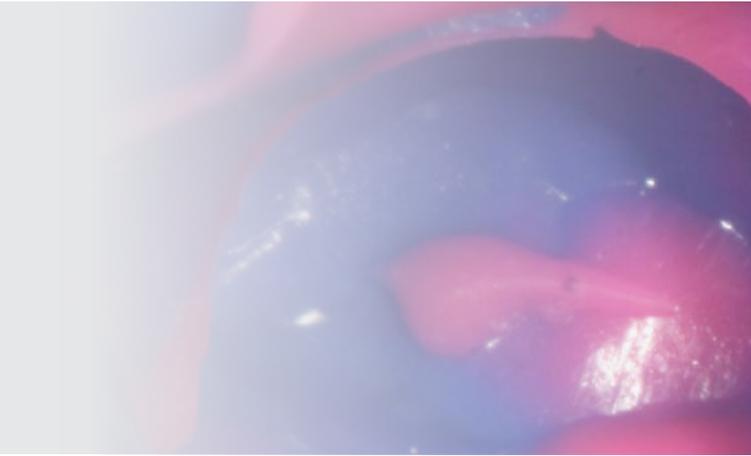

## HYDROPHILIA

Hydrophilia is another essential characteristic for an impression material as it makes a decisive contribution to the accurate reproduction of detail. The more hydrophilic a material is, the better able it is to flow into humid areas and copy surfaces accurately, with less risk of bubbles becoming incorporated.<sup>[5,6]</sup>

## TALKING ABOUT HYDROPHILIA

Not all impression materials behave in the same way in terms of hydrophilia.

Studies published in clinical literature have shown that the high hydrophilia of certain materials can result in the absorption of water and compromise dimensional accuracy.<sup>[7]</sup>

On the other hand, the hydrophobic nature of silicones does not result in any behaviour that is potentially detrimental to the accuracy of the prosthetic process. At the same time, the addition of surfactants to the formula also allows them to flow readily in wet environments.





## HYDROCOMPATIBILITY. MORE THAN HYDROPHILIA.

**Zhermack defines hydrocompatibility** as an affinity for water.

Zhermack has therefore elevated the concept of hydrophilia to a higher level. **Zhermack defines hydrocompatibility** as an affinity for water. Zhermack therefore uses the concept of **hydrocompatibility to differentiate its own silicones** from other materials on the market. Thanks to their **low angle of contact**, Zhermack silicones offer **high performance in humid environments** and maintain dimensional stability.

## A CHOICE OF QUALITY

Hydrorise has been shown to have one **of the best angles of contact** on the market.\* Its **excellent hydrocompatibility** helps obtain **precise and accurate impressions**.



\*In-house comparative tests against some of the best-known impression materials on the market.

# Hydrorise System

Everything contributes to accuracy.  
What more could you want?



## ALMOST 100% ELASTIC RECOVERY

Good elastic recovery is a fundamental characteristic for mixed impressions and those of natural abutments.<sup>[4]</sup> Hydrorise System products boast an **excellent elastic recovery** of at least **99%.\***

Material is therefore able to return to its original shape after the deformation caused by removing the impression from the oral cavity, contributing further to the accuracy of the impression.\*\*

## TEAR RESISTANCE

Impressions taken with any of the Hydrorise System viscosities resist tearing during removal from the mouth.



## ACCURATE EVEN DAYS LATER


With Hydrorise System, impressions do not need to be cast immediately: the dentist and dental technician therefore enjoy greater flexibility in impression management.

The **dimensional stability** of Hydrorise System helps maintain the accuracy of impressions **for up to 21 days.**

\* 99% for Hydrorise Putty and Maxi Putty and 99.5% for all other viscosities of Hydrorise System.

\*\* ISO 4823:2015

## Patient safety, dentist satisfaction

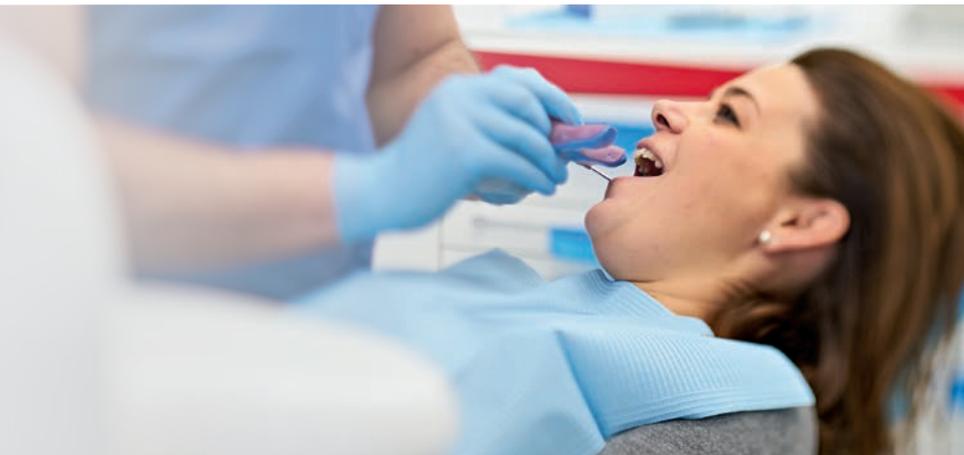

### BIOCOMPATIBLE, EVEN ON DAMAGED MUCOSA

For the professional, choosing a biocompatible material means choosing to operate safely, safeguarding the patient, and protecting him against irritation or sensitisation of the mucosae and oral tissues. It is also important to be able to count on a material presenting a low risk of allergic or toxic reactions.

The high **biocompatibility** of Hydrorise System permits its **use on healthy** and **damaged mucosa**, thus offering the best possible guarantee of safety.

### A SAFER CHOICE

Tested in compliance with the latest European medical device standards, Hydrorise System is:

NON-IRRITANT FOR THE ORAL MUCOSAE

NON-CYTOTOXIC

NON-SENSITISING

### Safe for use even on intolerant patients.

All Zhermack addition silicones **are gluten- and lactose-free**, which guarantees peace of mind and safety even when used on intolerant patients.

This allows the dentist to perform impression procedures with peace of mind and in absolute safety.



# A perfect combination

Hydrorise System and Sympress,  
the ideal combination for quality mixing.

## FOCUS

### A RELIABLE MACHINE

Hydrorise System can be used with **Sympress**, the automatic mixer designed for quick and easy mixing of impression materials in 5:1 cartridges.

#### VERSATILE

- Compatible with all the most common impression materials on the market (VPS and polyethers)
- Can be used with hard and soft cartridges (360 or 380 ml)

#### FUNCTIONAL

- Compact design occupies less worktop space
- Silent

#### EASY TO USE

- Two mixing speeds
- Constant and better quality mixing than manual mixing



# Quality mixing

With Zhermack, mixing becomes automatic to make your everyday work easier.

## WHY PREFER AUTOMATIC MIXING?

**Automatic mixing** improves impression quality compared to manual mixing and produces a **more homogeneous mix**. It reduces the risk of incorrect dosing and the incorporation of air bubbles in the mix. Automatic mixing also reduces impression material preparation times, even in the hands of less expert users, which in turn saves time and affords the user greater comfort. <sup>[8,9]</sup>

**Zhermack's 5:1 system, even better performance.**



**Dynamic-static tips  
reduce material waste  
by up to 22%\***

\*Compared to the most commonly used mixing tips of our competitors.



Cartridges are easy to insert in the machine and come ready for use

The mixing tip locker ensures quick and secure fixing

ZHERMACK'S 380 ML  
CARTRIDGES ARE  
COMPATIBLE WITH MOST  
COMMON MIXERS  
ON THE MARKET

# Clinical case

A clinical case of the complete rehabilitation of a patient's dental arches. **Hydrorise Implant** was used for implant prosthodontic purposes in the lower arch while **Hydrorise** was used in the upper arch for the prosthodontic treatment of natural teeth.




1. Baseline




2. Implants in position




3. Pick-up in position

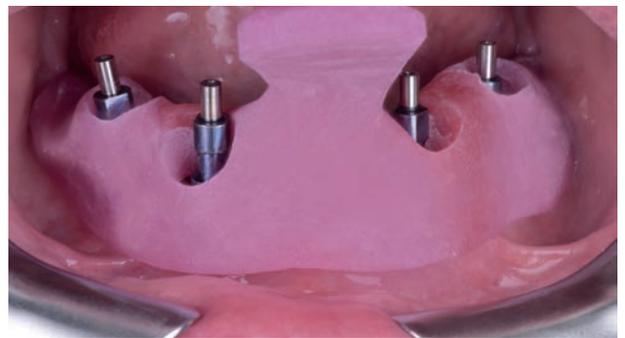


4. In-mouth testing of custom impression tray

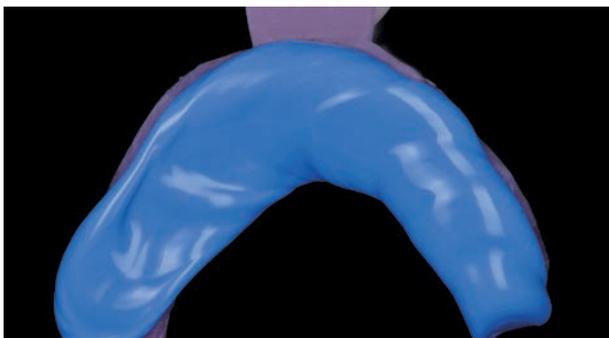

5. Hydrorise Implant Medium Body on the custom impression tray

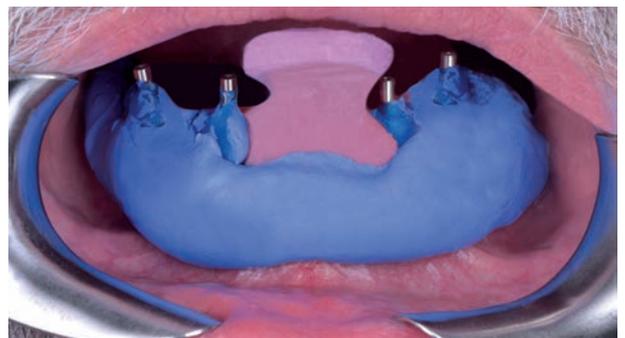

6. The Hydrorise Implant Medium Body impression in the patient's mouth

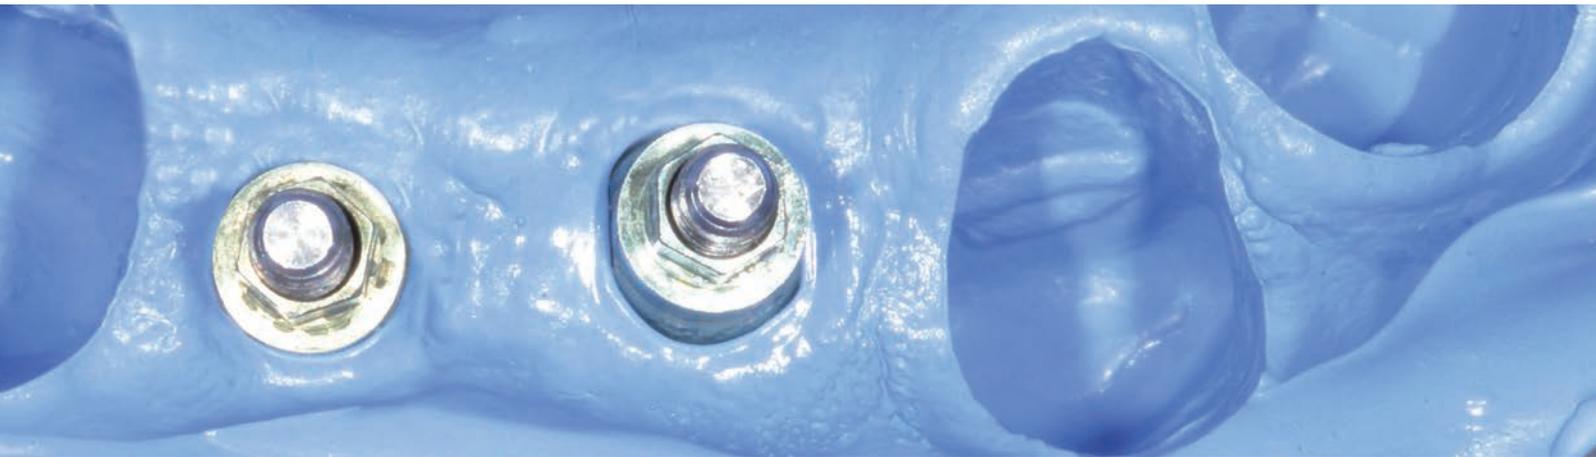

7. The Hydrorise Implant Medium Body impression



8. Preparation of the upper arch teeth



9. Insertion of the displacement cords



10. Positioning Hydrorise Light Body on the upper arch abutments



11. Upper arch impression of natural abutments taken with Hydrorise Heavy Body and Light Body



12. The patient's smile at the end of the treatment

# technical data



| HYDRORISE SYSTEM                | Delivery System           | Type of setting | Working time, including mixing time* (min:s) | Time in mouth** (min:s) | Setting time* (min:s) | Hardness Shore A |
|---------------------------------|---------------------------|-----------------|--|-------------------------|-----------------------|------------------|
| <b>Hydrorise Putty</b>          | Manual mixing             | Normal Set      | 2:00   | 3:30                    | 5:30                  | 60 ± 2           |
|                                 |                           | Fast Set        | 1:30   | 2:30                    | 4:00                  |                  |
| <b>Hydrorise Maxi Putty</b>     | 5:1 automatic mixing      | Normal Set      | 2:00   | 3:30                    | 5:30                  | 60 ± 2           |
|                                 |                           | Fast Set        | 1:30   | 2:30                    | 4:00                  |                  |
| <b>Hydrorise Implant Heavy</b>  | 5:1 automatic mixing      | Normal Set      | 2:00   | 3:30                    | 5:30                  | 65               |
| <b>Hydrorise Heavy</b>          | 1:1 semi-automatic mixing | Normal Set      | 2:00   | 3:30                    | 5:30                  | 60 ± 2           |
|                                 |                           | Fast Set        | 1:30   | 2:30                    | 4:00                  |                  |
| <b>Hydrorise Maxi Heavy</b>     | 5:1 automatic mixing      | Normal Set      | 2:00   | 3:30                    | 5:30                  | 60 ± 2           |
|                                 |                           | Fast Set        | 1:30   | 2:30                    | 4:00                  |                  |
| <b>Hydrorise Implant Medium</b> | 5:1 automatic mixing      | Normal Set      | 2:00   | 3:30                    | 5:30                  | 60               |
|                                 |                           | Quick Set       | 1:30   | 2:00                    | 3:30                  |                  |
| <b>Hydrorise Monophase</b>      | 1:1 semi-automatic mixing | Normal Set      | 2:00   | 3:30                    | 5:30                  | 54 ± 2           |
|                                 |                           | Fast Set        | 1:30   | 2:30                    | 4:00                  |                  |
| <b>Hydrorise Maxi Monophase</b> | 5:1 automatic mixing      | Normal Set      | 2:00   | 3:30                    | 5:30                  | 54 ± 2           |
|                                 |                           | Fast Set        | 1:30   | 2:30                    | 4:00                  |                  |
| <b>Hydrorise Regular</b>        | 1:1 semi-automatic mixing | Normal Set      | 2:00   | 3:30                    | 5:30                  | 45 ± 2           |
|                                 |                           | Fast Set        | 1:30   | 2:30                    | 4:00                  |                  |
| <b>Hydrorise Implant Light</b>  | 1:1 semi-automatic mixing | Normal Set      | 2:00   | 3:30                    | 5:30                  | 55               |
| <b>Hydrorise Light</b>          | 1:1 semi-automatic mixing | Normal Set      | 2:00   | 3:30                    | 5:30                  | 45 ± 2           |
|                                 |                           | Fast Set        | 1:30   | 2:30                    | 4:00                  |                  |
| <b>Hydrorise Extra Light</b>    | 1:1 semi-automatic mixing | Normal Set      | 2:00   | 3:30                    | 5:30                  | 45 ± 2           |
|                                 |                           | Fast Set        | 1:30   | 2:30                    | 4:00                  |                  |

\* Times are intended from the beginning of mixing at 23°C (73 °F).

\*\* Time in mouth is intended at 35°C / 95°F.

## Find out more about Zhermack impression products



## FOCUS

The disinfection of the impression is an essential step in order to limit the risk of cross-contamination between the dental practice and the dental laboratory.

All Zhermack silicones can be disinfected using products containing quaternary ammonium salts, mixtures of alcohol and surface tension reducers, such as **Zeta 7 Spray** and **Zeta 7 Solution** from Zhermack's Zeta Hygiene line, whilst maintaining their dimensional stability and surface detail reproduction even after disinfection<sup>[10,11]</sup>.



### **Zeta 7 Spray**

Ready-to-use disinfectant spray with a broad spectrum of action for rapid impression disinfection.

### **Zeta 7 Solution**

Concentrated disinfectant with a broad spectrum of action for impression disinfection.

# Codes and packaging



## extraPro

### HYDRORISE PUTTY - HIGH VISCOSITY ADDITION SILICONE

| Code    | Setting time | Packaging   |
|---------|--------------|---|
| C207010 | Normal Set   | 2 x 300 ml tubs (Base + Catalyst) + 2 measuring spoons  |
| C207011 | Fast Set     |   |
| C207012 | Normal Set   | Eco Pack: 2 x 900 ml tubs (Base + Catalyst) + 2 measuring spoons  |
| C207013 | Fast Set     |   |
| C207071 | Fast Set     | Mini Kit: 2 x 100 ml tubs (Base + Catalyst) of Putty Fast + 2 measuring spoons<br>1 x 50 ml cartridge (Base + Catalyst) of Light Fast + 6 mixing tips (small) |

### HYDRORISE MAXI PUTTY - HIGH VISCOSITY ADDITION SILICONE

| Code    | Setting time | Packaging   |
|---------|--------------|---|
| C207044 | Normal Set   | 2 x 380 ml cartridges (Base + Catalyst) + 15 dynamic-static mixing tips + 2 tip lockers |
| C207045 | Fast Set     |   |
| C207064 | Normal Set   | Eco Pack: 6 x 380 ml cartridges (Base + Catalyst) + 2 tip lockers                       |
| C207065 | Fast Set     |   |

### HYDRORISE IMPLANT HEAVY BODY - HIGH VISCOSITY ADDITION SILICONE

| Code    | Setting time | Packaging   |
|---------|--------------|---|
| C207090 | Normal Set   | 2 x 380 ml cartridges (Base + Catalyst) + 15 dynamic-static mixing tips + 2 tip lockers   |
| C207095 | Normal Set   | <b>Hydrorise Implant Kit Heavy/Light:</b><br>1 x 380 ml cartridge (Base + Catalyst) of Heavy Body + 1 x 50 ml cartridge (Base + Catalyst) of Light Body + 6 dynamic-static mixing tips + 6 mixing tips (small) + 1 tip locker |

### HYDRORISE HEAVY BODY - HIGH VISCOSITY ADDITION SILICONE

| Code    | Setting time | Packaging   |
|---------|--------------|---|
| C207008 | Normal Set   | 2 x 50 ml cartridges (Base + Catalyst) + 6 mixing tips (medium) |
| C207009 | Fast Set     |   |

### HYDRORISE MAXI HEAVY BODY - HIGH VISCOSITY ADDITION SILICONE

| Code    | Setting time | Packaging   |
|---------|--------------|---|
| C207042 | Normal Set   | 2 x 380 ml cartridges (Base + Catalyst) + 15 dynamic-static mixing tips + 2 tip lockers |
| C207043 | Fast Set     |   |
| C207062 | Normal Set   | Eco Pack: 6 x 380 ml cartridges (Base + Catalyst) + 2 tip lockers                       |
| C207063 | Fast Set     |   |

### HYDRORISE IMPLANT MEDIUM BODY - MEDIUM VISCOSITY ADDITION SILICONE

| Code    | Setting time | Packaging   |
|---------|--------------|---|
| C207092 | Normal Set   | 2 x 380 ml cartridges (Base + Catalyst) + 15 dynamic-static mixing tips + 2 tip lockers |
| C207122 | Quick Set    |   |
| C207096 | Normal Set   | 1 x 380 ml cartridge (Base + Catalyst) + 6 dynamic-static mixing tips + 1 tip locker    |
| C207126 | Quick Set    |   |

### HYDRORISE MONOPHASE - MEDIUM VISCOSITY ADDITION SILICONE

| Code    | Setting time | Packaging   |
|---------|--------------|---|
| C207006 | Normal Set   | 2 x 50 ml cartridges (Base + Catalyst) + 6 mixing tips (medium) |
| C207007 | Fast Set     |   |

### HYDRORISE MAXI MONOPHASE - MEDIUM VISCOSITY ADDITION SILICONE

| Code    | Setting time | Packaging   |
|---------|--------------|---|
| C207040 | Normal Set   | 2 x 380 ml cartridges (Base + Catalyst) + 15 dynamic-static mixing tips + 2 tip lockers |
| C207041 | Fast Set     |   |

### HYDRORISE REGULAR BODY - MEDIUM VISCOSITY ADDITION SILICONE

| Code    | Setting time | Packaging   |
|---------|--------------|---|
| C207004 | Normal Set   | 2 x 50 ml cartridges (Base + Catalyst) + 12 mixing tips (small) |
| C207005 | Fast Set     |   |

### HYDRORISE IMPLANT LIGHT BODY - LOW VISCOSITY ADDITION SILICONE

| Code    | Setting time | Packaging   |
|---------|--------------|---|
| C207091 | Normal Set   | 2 x 50 ml cartridges (Base + Catalyst) + 12 mixing tips (small)   |
| C207095 | Normal Set   | <b>Hydrorise Implant Kit Heavy/Light:</b><br>1 x 380 ml cartridge of Heavy Body + 1 x 50 ml cartridge of Light Body + 6 dynamic-static mixing tips + 6 mixing tips (small) + 1 tip locker |

### HYDRORISE LIGHT BODY - LOW VISCOSITY ADDITION SILICONE

| Code    | Setting time | Packaging  |
|---------|--------------|--|
| C207000 | Normal Set   | 2 x 50 ml cartridges (Base + Catalyst) + 12 mixing tips (small)  |
| C207001 | Fast Set     |  |
| C207071 | Normal Set   | Mini Kit: 2 x 100 ml tubs (Base + Catalyst) of Putty Fast + 2 measuring spoons + 1 x 50 ml cartridge (Base + Catalyst) of Light Fast + 6 mixing tips (small) |

### HYDRORISE EXTRA LIGHT BODY - LOW VISCOSITY ADDITION SILICONE

| Code    | Setting time | Packaging   |
|---------|--------------|---|
| C207002 | Normal Set   | 2 x 50 ml cartridges (Base + Catalyst) + 12 mixing tips (small) |
| C207003 | Fast Set     |   |

### Equipment

| Code      | Model                  |
|-----------|------------------------|
| 6000-0000 | Sympress – 230 V       |
| 6000-1000 | Sympress – 120 V       |
| 6000-2000 | Sympress 230 V UK plug |
| 6000-3000 | Sympress 100 V         |

For the full list of Sympress accessories visit [www.zhermack.com](http://www.zhermack.com)



### ACCESSORIES

| Code    | Product                       | Code    | Product                                |
|---------|-------------------------------|---------|--|
| C202085 | Mixing tips - small (48 pcs)  | C700025 | Universal Tray Adhesive - 10 ml bottle |
| C202086 | Mixing tips - medium (48 pcs) | C202100 | D2 1:1 dispenser                       |
| D510010 | Putty Cut                     | C205530 | Dynamic-static mixing tips (50 pcs)    |
| C202090 | Yellow oral tips (48 pcs)     | C205540 | Tip locker (2 pcs)                     |

## Bibliography

- [1] P. Baldissara , R. Meneghello , C. Parisi , A. M. Messias , F. Ghelli , L. Ciocca, HYPERLINK "https://cris.unibo.it/handle/11585/726162" Accuracy And Precision Of Impression Materials Designed For Implant Prosthodontics, in: IADR proceedings, 2019 (proceedings of the IADR/AADR/CADR 97TH GENERAL SESSION, Vancouver, BC, Canada, 19-22 June 2019) [Conference Proceedings-poster]
- [2] GAYATHRIDEVI, S. K., et al. Impression techniques in implants. Journal of Dental and Orofacial Research, 2016; 12.2: 11-19.
- [3] KURTULMUS-YILMAZ, Sevcn, et al. Digital evaluation of the accuracy of impression techniques and materials in angulated implants. Journal of dentistry, 2014, 42.12: 1551-1559. doi: 10.1016/j.jdent.2014.10.008
- [4] Shillingburg, Herbert T., et al. Fundamentals of fixed prosthodontics. Quintessence Publishing Company, 1997.
- [5] Nassar U, Tavoossi F, Pan Y W, Milavong-Viravongsa N, Heo G, Nychka J. Comparison of the contact angle of water on set elastomeric impression materials, J Can Dent Assoc 2018; 84: 1-7. ISSN: 1488-2159
- [6] Rubel B. Impression Materials: A Comparative Review of Impression Materials Most Commonly Used in Restorative Dentistry. Dental Clinics of North America. 2007; 51(3): 632 . DOI: 10.1016/j.cden.2007.03.006
- [7] Gonçalves F S, Popoff D A V, Castro C D L, Silva G C, Moreira A, Magalhães C S, Moreira A N. Dimensional stability of elastomeric impression materials: a critical review of the literature. The European journal of prosthodontics and restorative dentistry. 2011; 19:1-4. doi:10.1922/EJPRD\_998Silva04
- [8] Daou E. E, The elastomers for complete denture impression: A review of the literature. The Saudi Dental Journal. 2010; 22:153-160
- [9] Di Felice R, Scotti R, Belsler U. The influence of the mixing technique on the content of voids in two polyether impression materials. Schweiz Monatsschr Zahnmed. 2002; 112: 12-16
- [10] Sinobad T, Obradović-Đuričić K, Nikolić Z, Dodić S, Lazić V, Sinobad V, Jesenko-Rokvić A. The effect of disinfectants on dimensional stability of addition and condensation silicone impressions. Vojnosanitetski preglad, 2014, 71.3: 251-258.
- [11] Amin WM, Al-Ali MH, Al Tarawneh SK, Taha ST, Saleh MW, Ereifij N. The effects of disinfectants on dimensional accuracy and surface quality of impression materials and gypsum casts. J Clin Med Res. 2009;1(2):81-89. doi:10.4021/jocmr2009.04.1235

# Fulfilling your needs